

ANALIZA BIAŁEK



100013140

Laboratory of Analysis

Client: Chatlotte Redfern
Order number: 100016577
Name: BIOPURA ACETIC WATER
Number of samples: 1 vial

Batch number: AA101
Recive date: 2026-07-24
Start date: 2026-07-24
End date: 2026-07-24


Sample identification

Tests	Method of taking a sample	Form
Microbiological	Sample provided by customer	Transparent liquid in a glass vial

Results

Test	Sample name	Result
TYMC	BIOPURA ACETIC WATER 10ML	PASS
TAMC	BIOPURA ACETIC WATER 10ML	PASS
Presence of presumptive Escherichia Coli	BIOPURA ACETIC WATER 10ML	NOT DETECTED
Presence of Salmonella Spp.	BIOPURA ACETIC WATER 10ML	NOT DETECTED

Photo of the test sample

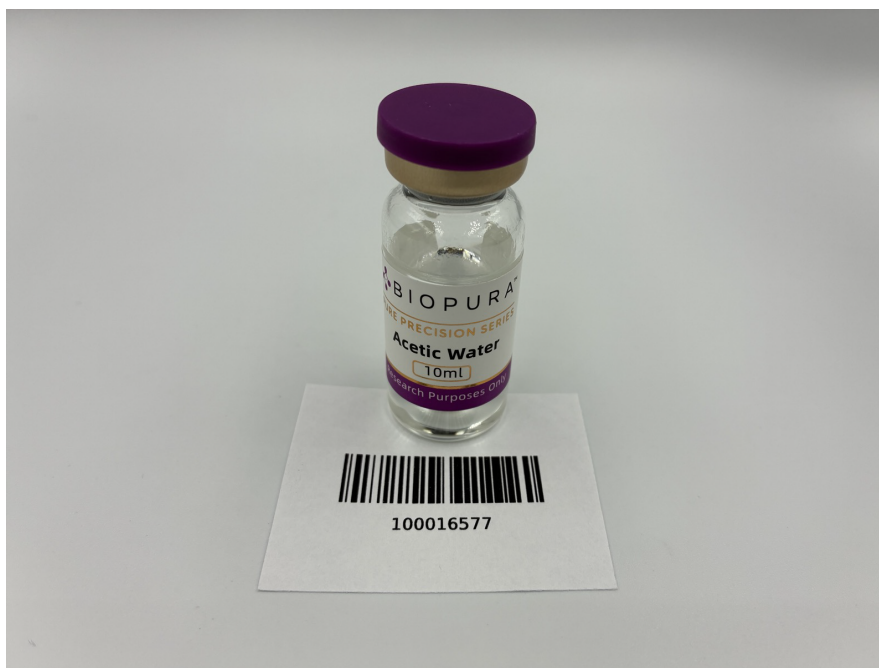

Password

F16J4K9Q

Analiza Białek sp. z o.o.
KRS: 0000966168
NIP: 8992922970
REGON: 521751875

Headquarters and Laboratory:
ul. Duńska 9, 54-427 Wrocław
Budynek DELTA

Lab technician:
Analysis and research specialist
mgr Arkadiusz Zajac